

A BINAURAL HEARING AID SYSTEM WITH COORDINATED SOUND PROCESSING

FIELD OF THE INVENTION

The present invention relates to a binaural hearing aid system with a first hearing aid and a
5 second hearing aid, each of which comprises a microphone, an A/D converter for provision
of a digital input signal in response to sound signals received at the respective microphone
in a sound environment, a processor that is adapted to process the digital input signals in
accordance with a predetermined signal processing algorithm to generate a processed
output signal, and a D/A converter and an output transducer for conversion of the
10 respective processed sound signal to an acoustic output signal.

BACKGROUND OF THE INVENTION

Today's conventional hearing aids typically comprise a Digital Signal Processor (DSP) for
processing of sound received by the hearing aid for compensation of the user's hearing
loss. As is well known in the art, the processing of the DSP is controlled by a signal
15 processing algorithm having various parameters for adjustment of the actual signal
processing performed. The gains in each of the frequency channels of a multi-channel
hearing aid are examples of such parameters.

The flexibility of the DSP is often utilized to provide a plurality of different algorithms and/or
a plurality of sets of parameters of a specific algorithm. For example, various algorithms
20 may be provided for noise suppression, i.e. attenuation of undesired signals and
amplification of desired signals. Desired signals are usually speech or music, and
undesired signals can be background speech, restaurant clatter, music (when speech is
the desired signal), traffic noise, etc.

The different algorithms or parameter sets are typically included to provide comfortable and
25 intelligible reproduced sound quality in different sound environments, such as speech,
babble speech, restaurant clatter, music, traffic noise, etc. Audio signals obtained from
different sound environments may possess very different characteristics, e.g. average and
maximum sound pressure levels (SPLs) and/or frequency content. Therefore, in a hearing
aid with a DSP, each type of sound environment may be associated with a particular
30 program wherein a particular setting of algorithm parameters of a signal processing
algorithm provides processed sound of optimum signal quality in a specific sound
environment. A set of such parameters may typically include parameters related to
broadband gain, corner frequencies or slopes of frequency-selective filter algorithms and

parameters controlling e.g. knee-points and compression ratios of Automatic Gain Control (AGC) algorithms.

Consequently, today's DSP based hearing instruments are usually provided with a number of different programs, each program tailored to a particular sound environment category and/or particular user preferences. Signal processing characteristics of each of these
5 programs is typically determined during an initial fitting session in a dispenser's office and programmed into the instrument by activating corresponding algorithms and algorithm parameters in a non-volatile memory area of the hearing aid and/or transmitting corresponding algorithms and algorithm parameters to the non-volatile memory area.

10 Some known hearing aids are capable of automatically classifying the user's sound environment into one of a number of relevant or typical everyday sound environment categories, such as speech, babble speech, restaurant clatter, music, traffic noise, etc.

Obtained classification results may be utilised in the hearing aid to automatically select signal processing characteristics of the hearing aid, e.g. to automatically switch to the most
15 suitable algorithm for the environment in question. Such a hearing aid will be able to maintain optimum sound quality and/or speech intelligibility for the individual hearing aid user in various sound environments.

US 5,687,241 discloses a multi-channel DSP based hearing instrument that utilises continuous determination or calculation of one or several percentile values of input signal
20 amplitude distributions to discriminate between speech and noise input signals. Gain values in each of a number of frequency channels are adjusted in response to detected levels of speech and noise.

However, it is often desirable to provide a more subtle characterization of a sound environment than only discriminating between speech and noise. As an example, it may be
25 desirable to switch between an omni-directional and a directional microphone preset program in dependence of, not just the level of background noise, but also on further signal characteristics of this background noise. In situations where the user of the hearing aid communicates with another individual in the presence of the background noise, it would be beneficial to be able to identify and classify the type of background noise. Omni-directional
30 operation could be selected in the event that the noise being traffic noise to allow the user to clearly hear approaching traffic independent of its direction of arrival. If, on the other hand, the background noise was classified as being babble-noise, the directional listening program could be selected to allow the user to hear a target speech signal with improved signal-to-noise ratio (SNR) during a conversation.

Applying Hidden Markov Models for analysis and classification of the microphone signal may obtain a detailed characterisation of e.g. a microphone signal. Hidden Markov Models are capable of modelling stochastic and non-stationary signals in terms of both short and long time temporal variations. Hidden Markov Models have been applied in speech
5 recognition as a tool for modelling statistical properties of speech signals. The article "A Tutorial on Hidden Markov Models and Selected Applications in Speech Recognition", published in Proceedings of the IEEE, VOL 77, No. 2, February 1989 contains a comprehensive description of the application of Hidden Markov Models to problems in speech recognition.

- 10 WO 01/76321 discloses a hearing aid that provides automatic identification or classification of a sound environment by applying one or several predetermined Hidden Markov Models to process acoustic signals obtained from the listening environment. The hearing aid may utilise determined classification results to control parameter values of a signal processing algorithm or to control switching between different algorithms so as to optimally adapt the
15 signal processing of the hearing aid to a given sound environment.

The different available signal processing algorithms may change the signal characteristics significantly. In binaural hearing aid systems, it is therefore important that the determination of sound environment does not differ for the two hearing aids. However, since sound characteristics may differ significantly at the two ears of a user, it will often occur that sound
20 environment determination at the two ears of a user differs, and this leads to undesired different signal processing of sounds for each of the ears of the user.

SUMMARY OF THE INVENTION

Thus, there is a need for a binaural hearing aid system wherein sound environment determination does not differ for the two hearing aids so that signal processing in the two
25 hearing aids may be coordinated and the user be provided with desired processed sound in both ears at the same time.

According to the present invention, this and other objects are solved by provision of a binaural hearing aid system of the above-mentioned type wherein the hearing aids are connected either by wire or by a wireless link to at least one binaural sound environment
30 detector for binaural determination of the sound environment surrounding a user of the binaural hearing aid system based on at least one signal from the first hearing aid and at least one signal from the second hearing aid whereby the sound environment is determined and classified based on binaural signals. The one or more binaural sound environment detectors provide outputs for each of the first and second hearing aids for selection of the

signal processing algorithm of each of the hearing aid processors so that the hearing aids of the binaural hearing aid system perform coordinated sound processing.

In this way both hearing aids may process sound in response to a common determination of sound environment. Sound environment determination may be performed by one
5 common environment detector, for example situated in one of the hearing aids or in a remote control, or, by a plurality of environment detectors, such as an environment detector in each of the first and second hearing aids.

In the event that the user has substantially the same hearing loss in both ears and the sound environment is omni-directional, i.e. the sound environment does not change with
10 direction, coordination of sound processing in the hearing aids leads to execution of identical signal processing algorithms in the respective signal processors of the hearing aids. In the event that the hearing aid user suffers from a binaural hearing loss, the signal processing algorithms may desirably differ for compensation of the different binaural hearing losses.

15 It is an important advantage of the present invention that binaural sound environment detection is more accurate than monaural detection since signals from both ears are taken into account.

It is a further advantage of the present invention that signal processing in the hearing aids of the binaural hearing aid system is coordinated since the sound environment detection is
20 the same for both hearing aids.

BRIEF DESCRIPTION OF THE DRAWINGS

For a better understanding of the present invention reference will now be made, by way of example, to the accompanying drawings, in which:

25 Fig. 1 illustrates schematically a prior art monaural hearing aid with sound environment classification,

Fig. 2 illustrates schematically a first embodiment of the present invention,

Fig. 3 illustrates schematically a second embodiment of the present invention,

Fig. 4 illustrates schematically a third embodiment of the present invention, and

Fig. 5 illustrates schematically a fourth embodiment of the present invention.

DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

Fig. 1 illustrates schematically a prior art monaural hearing aid 10 with sound environment classification.

The monaural hearing aid 10 comprises a first microphone 12 and a first A/D converter (not shown) for provision of a digital input signal 14 in response to sound signals received at the microphone 12 in a sound environment, and a second microphone 16 and a second A/D converter (not shown) for provision of a digital input signal 18 in response to sound signals received at the microphone 16, a processor 20 that is adapted to process the digital input signals 14, 18 in accordance with a predetermined signal processing algorithm to generate a processed output signal 22, and a D/A converter (not shown) and an output transducer 24 for conversion of the respective processed sound signal 22 to an acoustic output signal.

The hearing aid 10 further comprises a sound environment detector 26 for determination of the sound environment surrounding a user of the hearing aid 10. The determination is based on the output signals of the microphones 12, 16. Based on the determination, the sound environment detector 26 provides outputs 28 to the hearing aid processor 20 for selection of the signal processing algorithm appropriate in the determined sound environment. Thus, the hearing aid processor 20 is automatically switched to the most suitable algorithm for the determined environment whereby optimum sound quality and/or speech intelligibility is maintained in various sound environments.

The signal processing algorithms of the processor 20 may perform various forms of noise reduction and dynamic range compression as well as a range of other signal processing tasks.

The sound environment detector 26 comprises a feature extractor 30 for determination of characteristic parameters of the received sound signals. The feature extractor 30 maps the unprocessed sound inputs 14, 18 sound features, i.e. the characteristic parameters. These features can be signal power, spectral data and other well-known features.

The sound environment detector 26 further comprises an environment classifier 32 for categorizing the sound environment based on the determined characteristic parameters. The environment classifier categorizes the sounds into a number of environmental classes, such as speech, babble speech, restaurant clatter, music, traffic noise, etc. The classification process may consist of a simple nearest neighbour search, a neural network, a Hidden Markov Model system or another system capable of pattern recognition. The output of the environmental classification can be a "hard" classification containing one

single environmental class or a set of probabilities indicating the probabilities of the sound belonging to the respective classes. Other outputs may also be applicable.

The sound environment detector 26 further comprises a parameter map 34 for the provision of outputs 28 for selection of the signal processing algorithms.

- 5 The parameter map 34 maps the output of the environment classification 32 to a set of parameters for the hearing aid sound processor 20. Examples of such parameters are amount of noise reduction, amount of gain and amount of HF gain. Other parameters may be included.

Figs. 2-5 illustrate various preferred embodiments of the present invention. The illustrated
10 binaural hearing aid system 1 comprises a first hearing aid 10 and a second hearing aid 10', each of which comprises a first microphone 12, 12' and an A/D converter (not shown) and a second microphone 16, 16' and A/D converter (not shown) for provision of a digital input signals 14, 14', 18, 18' in response to sound signals received at the respective microphones 12, 12', 16, 16' in a sound environment, a processor 20, 20' that is adapted to
15 process the digital input signals 14, 18, 14', 18' in accordance with a predetermined signal processing algorithm to generate a processed output signal 22, 22', and a D/A converter (not shown) and an output transducer 24, 24' for conversion of the respective processed sound signals 22, 22' to an acoustic output signal

In the embodiments illustrated in Figs. 2-4, each of the hearing aids 10, 10' of the binaural
20 hearing aid system 1 further comprises a binaural sound environment detector 26, 26' for determination of the sound environment surrounding a user of the binaural hearing aid system 1. The determination is based on the output signals of the microphones 12, 12', 16, 16'. Based on the determination, the binaural sound environment detector 26, 26' provides outputs 28, 28' to the hearing aid processors 20, 20' for selection of the signal processing
25 algorithm appropriate in the determined sound environment. Thus, the binaural sound environment detectors 26, 26' determines the sound environment based on signals from both hearing aids, i.e. binaurally, whereby hearing aid processors 20, 20' is automatically switched in co-ordination to the most suitable algorithm for the determined environment whereby optimum sound quality and/or speech intelligibility is maintained in various sound
30 environments by the binaural hearing aid system 1.

The binaural sound environment detectors 26, 26' illustrated in Figs. 2-4 are both similar to the binaural sound environment detector shown in Fig. 1 apart from the fact that the monaural environment detector only receives inputs from one hearing aid while each of the binaural sound environment detectors 26, 26' receives inputs from both hearing aids. Thus,

according to the present invention, signals are transmitted between the hearing aids 10, 10' so that the algorithms executed by the signal processors 20, 20' are selected in co-ordination, e.g. in case of an omni-directional sound environment, i.e. the sound environment does not change with direction, the algorithms are selected to be identical
5 apart from possible differences in hearing loss compensation of the two ears.

In the embodiment of Fig. 2, the unprocessed signals 14, 14', 18, 18' from the microphones 12, 12', 16, 16' of one hearing aid 10, 10' are transmitted to the other hearing aid and inputted to the respective feature extractor 30, 30'. Thus, feature extraction in each of the hearing aids is based on the identical four input signals so that identical sound environment
10 characteristic parameters will be determined binaurally in both hearing aids 10, 10'.

The signals may be transmitted in analogue form or in digital form, and the communication channel may be wired or wireless.

In the embodiment shown in Fig. 3, the output 36, 36' of the feature extractor 30, 30' of one hearing aid 10, 10' is transmitted to the respective other hearing aid 10', 10. The
15 environment classifier 32, 32' then operates on two sets of features 36, 36' to determine the environment. Since both environment classifiers 32, 32' receive the same data, they will produce the same output.

In the embodiment shown in Fig. 4, the output 38, 38' of the environment classifier 32, 32' of one hearing aid 10, 10' is transmitted to the respective other hearing aid 10, 10'. The
20 parameter map 34, 34' then operates on two inputs 38, 38' to produce the parameters for the processor algorithms, but since both parameter mapping units 34, 34' receive identical inputs, identical parameter values will be produced.

This embodiment has a number of advantages: Usually classification systems take both past and present data into account – they have memory. This makes them sensitive to
25 missing data, since a classification requires a complete data set. Therefore it is required that the data link is safe, in the sense that data is guaranteed to be transmitted. The parameter mapping can be implemented without memory so that only present data is taken into account when generating parameters. This makes the system robust to packet loss and latency, since the parameter mapping may simply re-use old data in the event that
30 data is missing. This will of course delay the correct action, but to the user the systems will appear to be synchronized.

The transmission data rate is low, since only a set of probabilities or logic values for the environment classes has to be transmitted.

Rather high latency can be accepted. By applying time constants to the variables that will change according to the output of the parameter mapping it is possible to smooth out any differences that is caused by latency. As described earlier it is important that signal processing in the two hearing instruments is coordinated. However if transition periods of a few seconds are allowed the system can operate with only 3-4 transmissions per second. Hereby, power consumption is kept low.

A binaural hearing aid system 1 with a remote control 40 is shown in Fig. 5. The environment detector 26 is positioned in the remote control 40. The required signals are transmitted to and from both hearing aids.

CLAIMS

1. A binaural hearing aid system comprising
a first hearing aid and a second hearing aid, each of which comprises
 - 5 a microphone and an A/D converter for provision of a digital input signal in response to sound signals received at the respective microphone in a sound environment,
 - a processor that is adapted to process the digital input signals in accordance with a predetermined signal processing algorithm to generate a processed output signal, and
 - 10 a D/A converter and an output transducer for conversion of the respective processed sound signal to an acoustic output signal, and
a binaural sound environment detector for binaural determination of the sound environment surrounding a user of the binaural hearing aid system based on at least one signal from the first hearing aid and at least one signal from the second hearing aid for provision of outputs
15 for each of the first and second hearing aids for selection of the signal processing algorithm of each of the respective hearing aid processors so that the hearing aids of the binaural hearing aid system perform coordinated sound processing.
2. A system according to claim 1, wherein the binaural sound environment detector having inputs for each of the digital input signals is provided in a remote control of the system.
- 20 3. A system according to claim 1, wherein the binaural sound environment detector is provided in one of the hearing aids and provides an output for the other hearing aid.
4. A system according to claim 1, wherein each of the hearing aids comprises a binaural sound environment detector.
5. A system according to any of the preceding claims, wherein the binaural sound
25 environment detector comprises
 - a feature extractor for determination of characteristic parameters of the received sound signals,
 - an environment classifier for categorizing the sound environment based on the determined characteristic parameters, and
 - 30 a parameter map for the provision of outputs for selection of the signal processing algorithms.

6. A system according to claim 4 and 5, wherein each of the feature extractors has inputs for each of the digital input signals.
7. A system according to claim 4 and 5, wherein each of the environment classifiers has inputs connected to each of the feature extractors.
- 5 8. A system according to claim 4 and 5, wherein each of the parameter maps has inputs for connected to each of the environment classifiers.

1/5

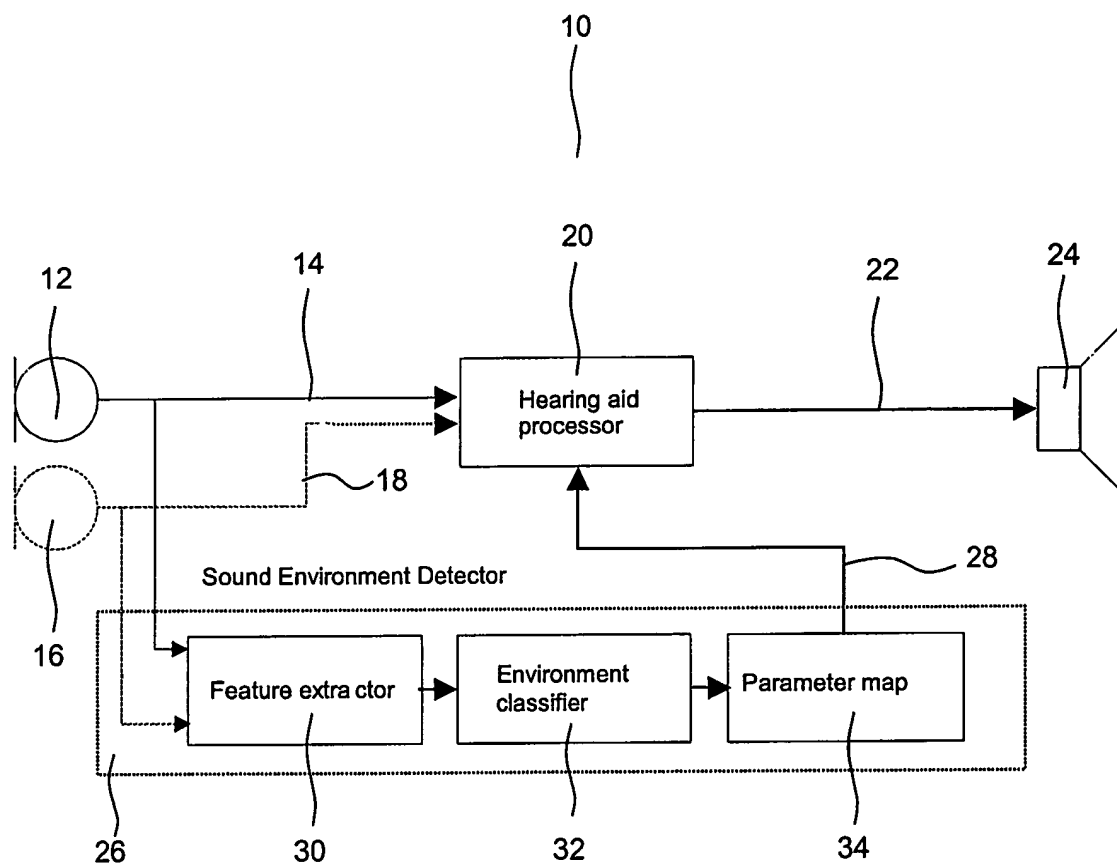


Fig. 1

2/5

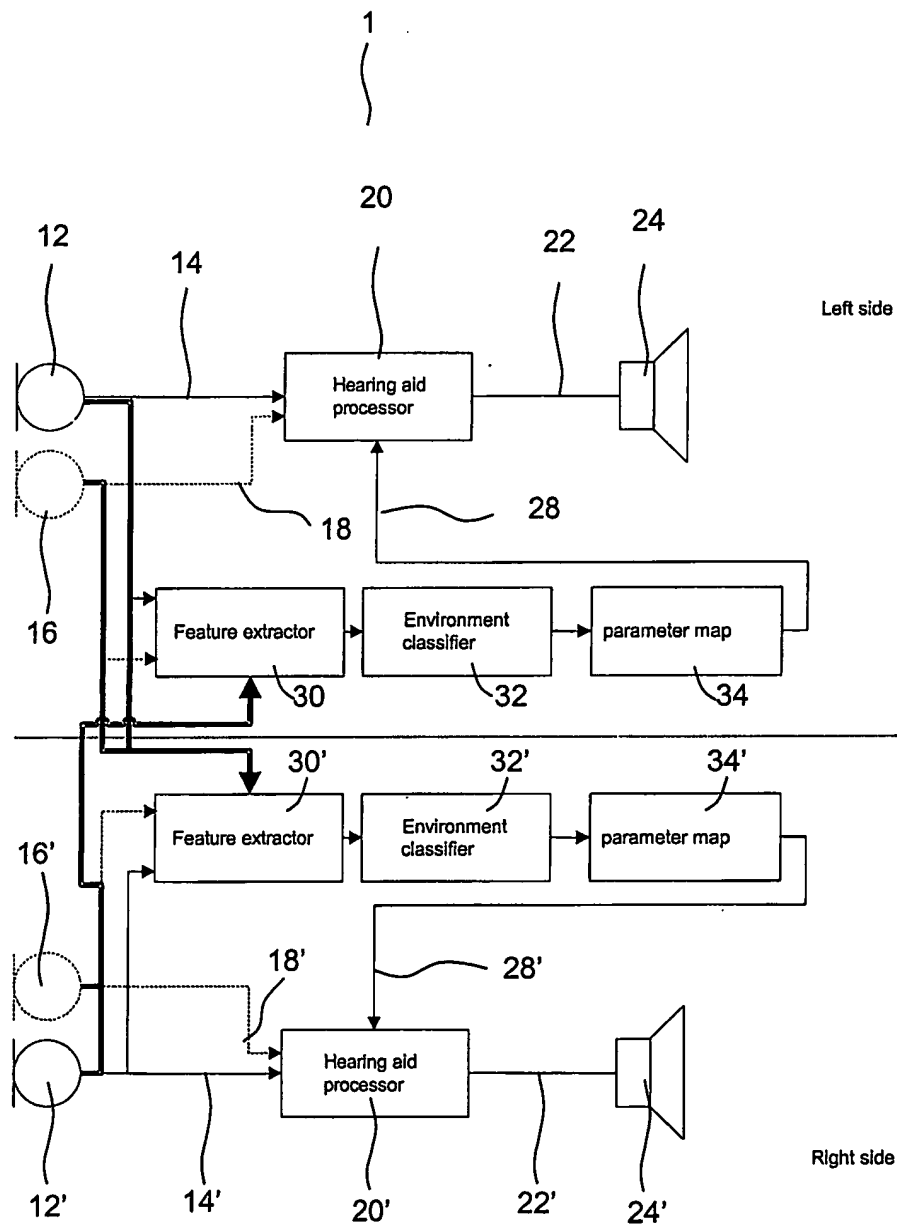


Fig. 2

3/5

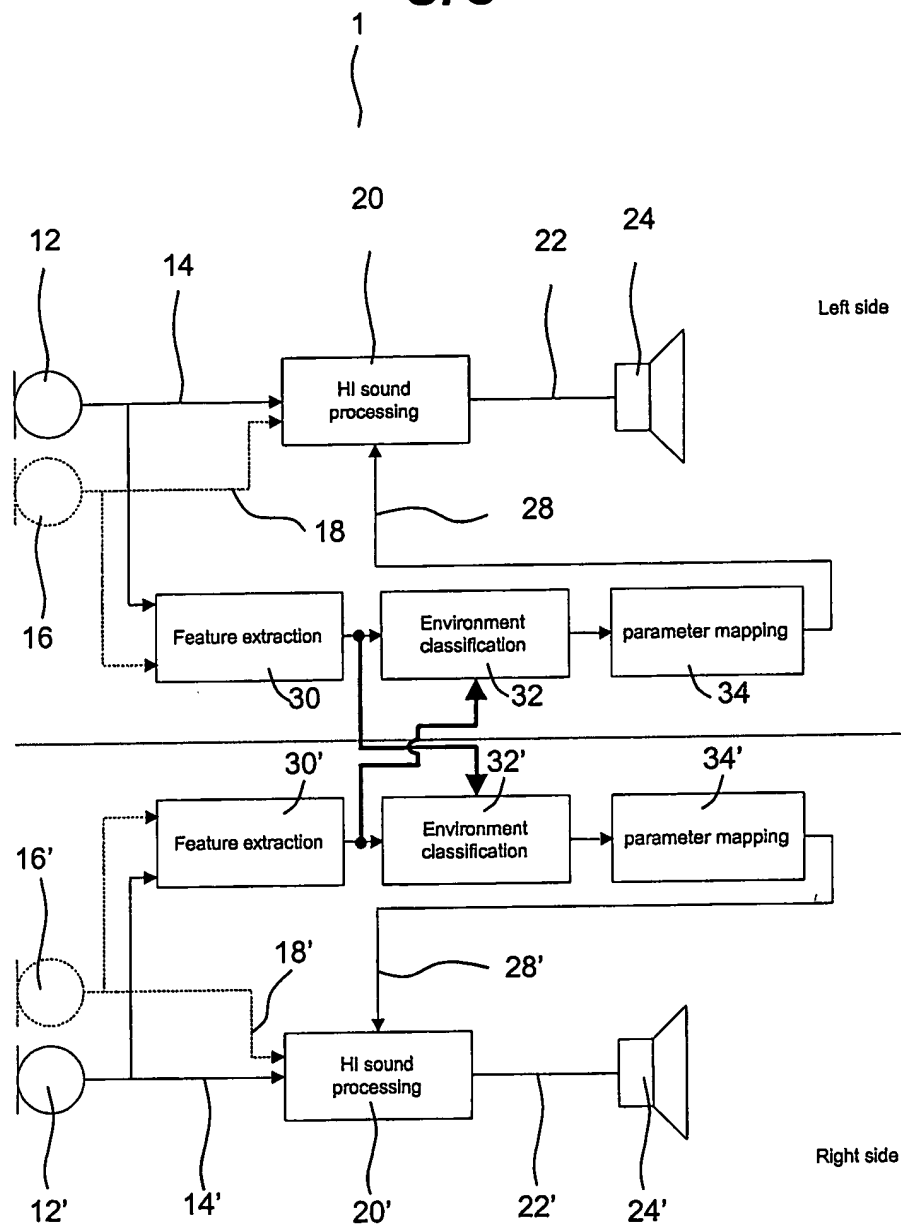


Fig. 3

4/5

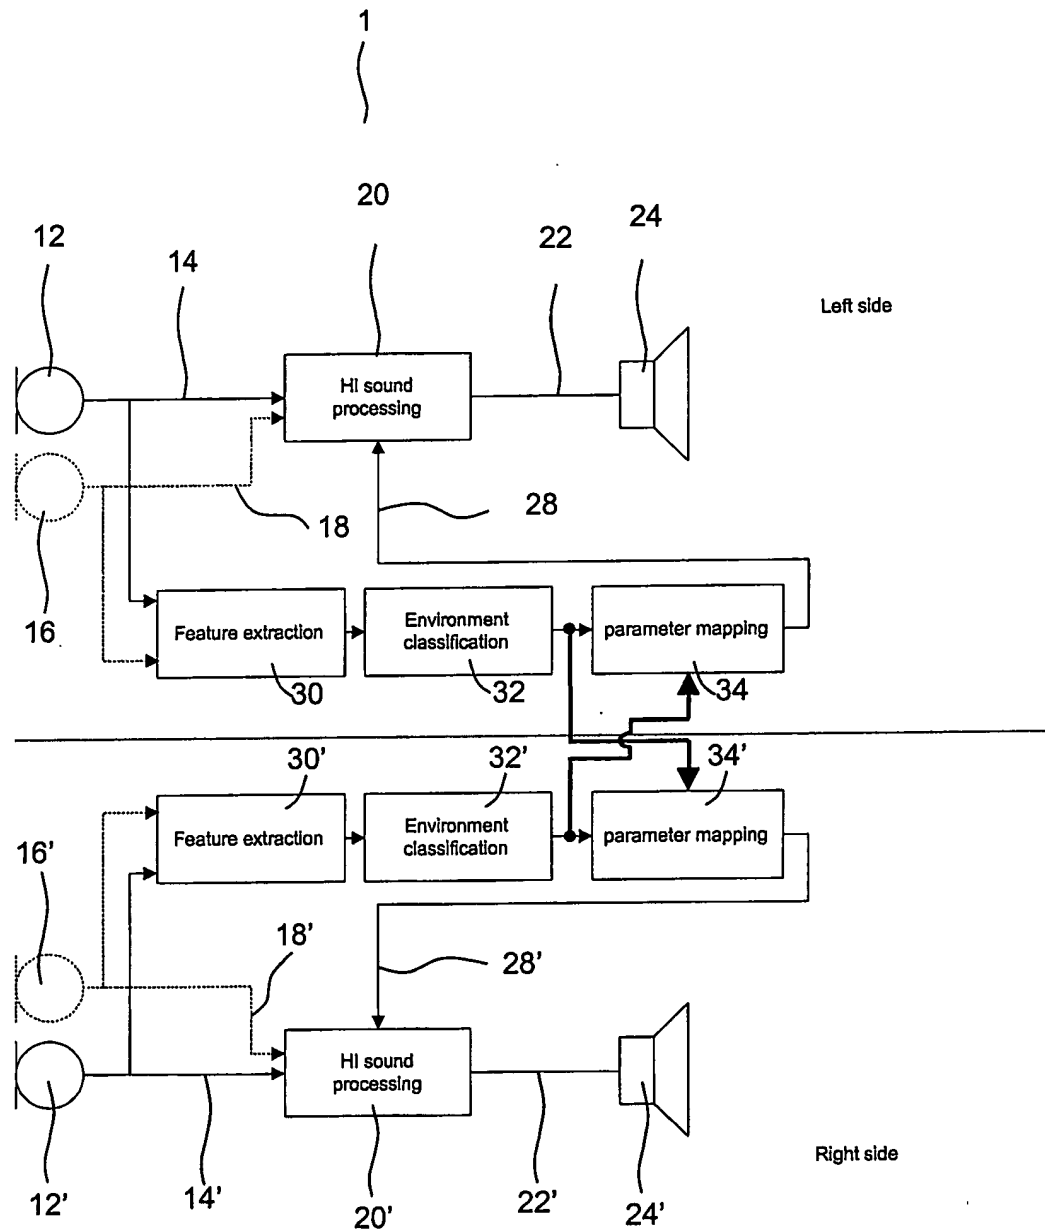


Fig. 4

5/5

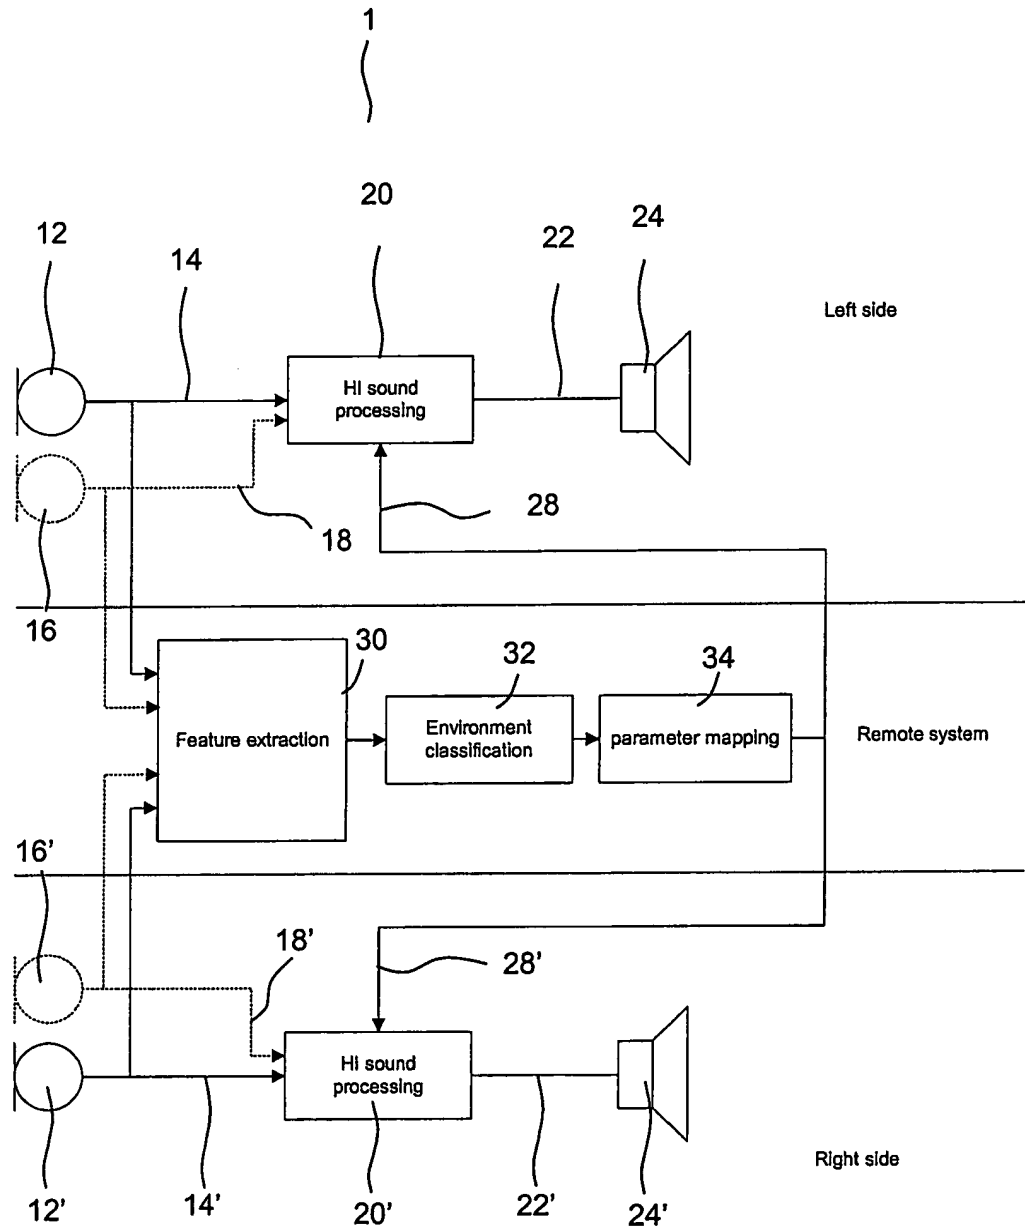


Fig. 5

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 H04R25/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 H04R

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 02/28143 A (SIEMENS AUDIOLOGISCHE TECHNIK ; NIEDERDRAENK TORSTEN (DE)) 4 April 2002 (2002-04-04) the whole document	1-8
X	US 5 757 932 A (BISGAARD NIKOLAI ET AL) 26 May 1998 (1998-05-26) the whole document	1-8
A	US 6 549 633 B1 (WESTERMANN SOEREN ERIK) 15 April 2003 (2003-04-15) the whole document	1-8
A	US 2002/037087 A1 (ALLEGRO SYLVIA ET AL) 28 March 2002 (2002-03-28) the whole document	5
A	WO 02/32208 A (PHONAK AG ; ALLEGRO SILVIA (CH)) 25 April 2002 (2002-04-25)	



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents :

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

Z document member of the same patent family

Date of the actual completion of the international search

9 November 2004

Date of mailing of the international search report

18/11/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Fülöp, I

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/DK2004/000442

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 0228143	A	04-04-2002	DE 10048354 A1	08-05-2002
			CN 1470149 T	21-01-2004
			WO 0228143 A2	04-04-2002
			EP 1360870 A2	12-11-2003
			US 2004013280 A1	22-01-2004
US 5757932	A	26-05-1998	US 5479522 A	26-12-1995
			AU 7248796 A	30-04-1997
			DE 69631781 D1	08-04-2004
			DK 855130 T3	12-07-2004
			EP 0855130 A1	29-07-1998
			NO 981559 A	08-06-1998
			WO 9714268 A1	17-04-1997
US 6549633	B1	15-04-2003	WO 9943185 A1	26-08-1999
			AU 733433 B2	17-05-2001
			AU 5982598 A	06-09-1999
			CA 2311405 A1	26-08-1999
			EP 1057367 A1	06-12-2000
			JP 2002504794 T	12-02-2002
US 2002037087	A1	28-03-2002	WO 0120965 A2	29-03-2001
			US 2002090098 A1	11-07-2002
			AU 2139901 A	24-04-2001
			CA 2400104 A1	29-03-2001
			EP 1348315 A2	01-10-2003
			JP 2004500592 T	08-01-2004
WO 0232208	A	25-04-2002	WO 0232208 A2	25-04-2002
			AU 2472202 A	29-04-2002
			CA 2439427 A1	25-04-2002
			EP 1470735 A2	27-10-2004